


# Peak Magnetic Field Comparison of AffloVest® and Monarch® HFCWO Vest

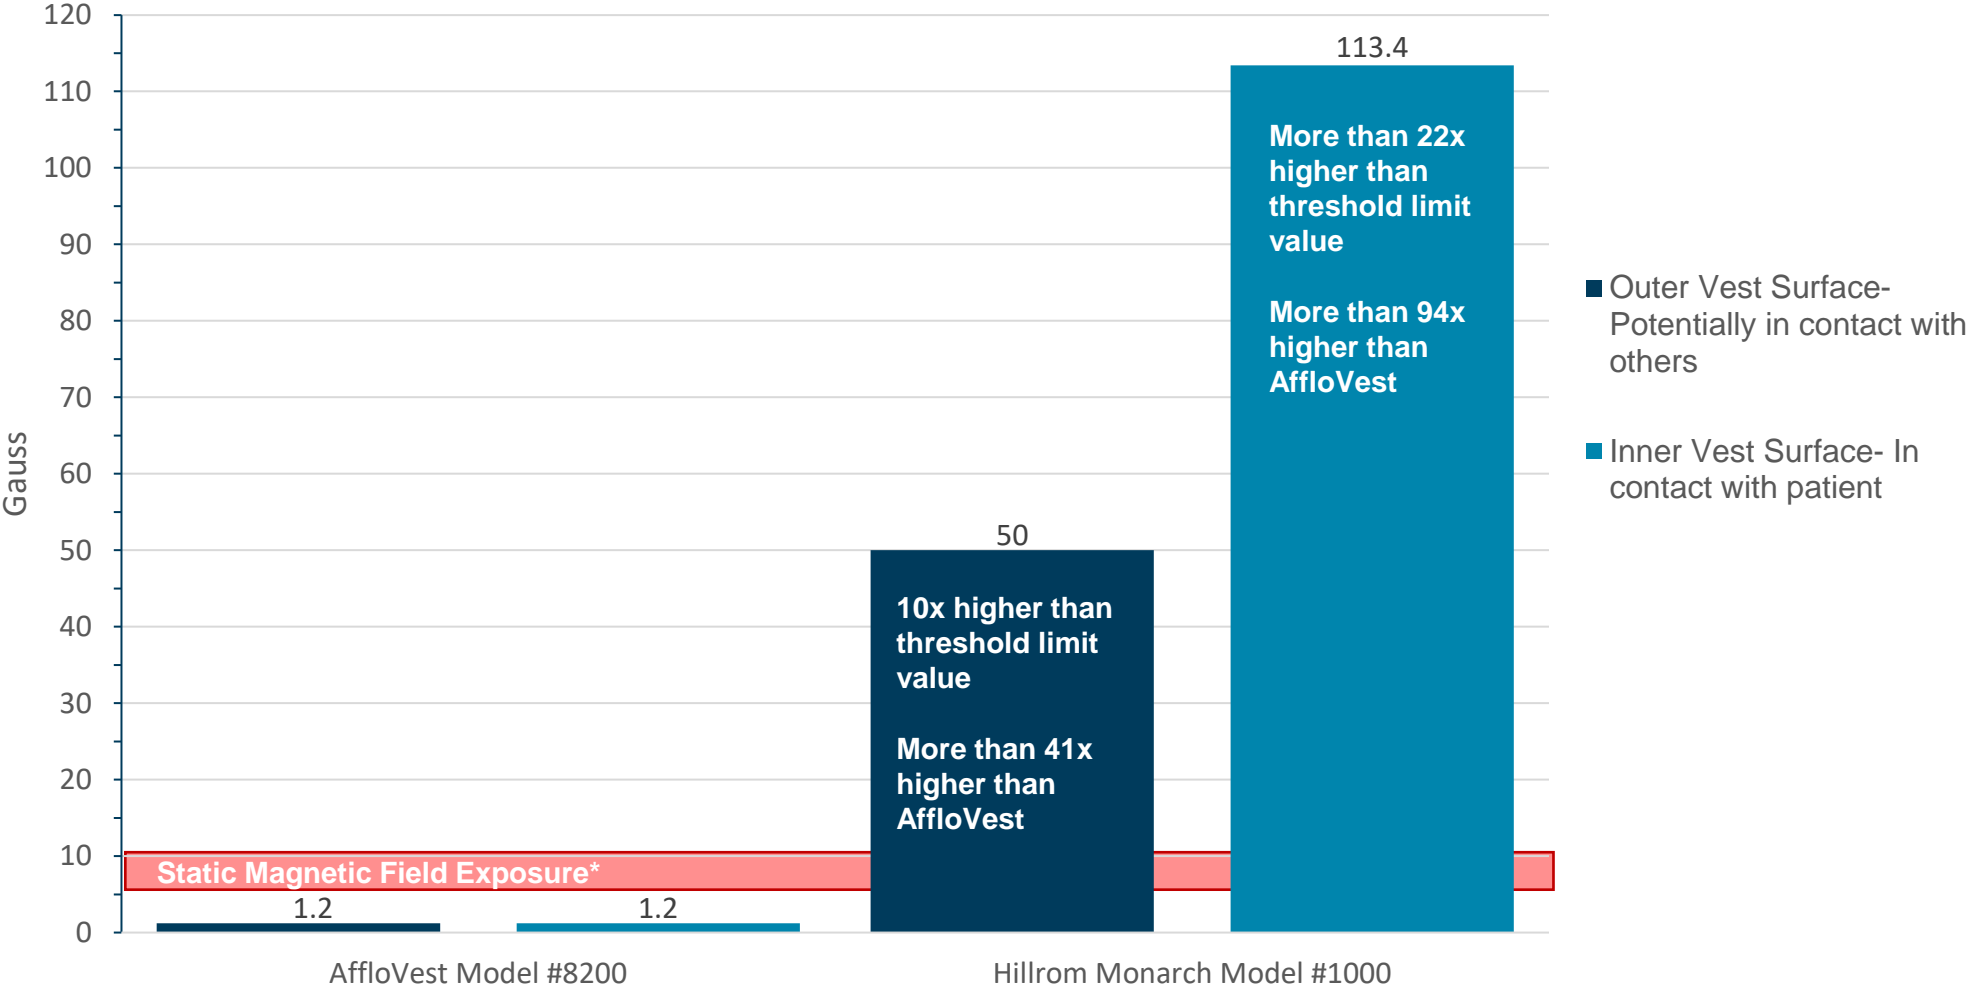

\*10G- Threshold at which the magnetic field may potentially impact pacemaker function  
 \*5G- Threshold limit value for medical device wearers and implanted medical devices including pacemakers

AffloVest is a registered trademark of Tactile Medical. Other marks are owned by respective companies. Data on file from F2 Labs, an independent 3<sup>rd</sup> party accredited testing laboratory.